

Certificate of Analysis - Amended Fast Track Distribution Lot

Product Description	ES02 NSCB FT Distribution lot					
Cell Line Provider	ES Cell International (Singapore)					
Distribution Lot Number	ES02-FTDL-1					
Date Vialed	13-June-2008					
Passage Number	63					
Culture Method	SOP-CC-020B, SOP-CC-030C, SOP-CC-037A,					
	SOP-CC-001B, SOP-CC-022B					
Cryopreservation Method	SOP-CC-035D					

The following testing specifications have been met for the specified product lot:

Test Description	Test Method	Test Specification	Result
Post-Thaw Viable Cell Recovery	SOP-CH-305A	Viable cells recovered	Pass
Identity by STR	SOP-CH-302B	Positive identity	Pass
Sterility	SOP-CH-304A	No contamination detected	Pass
Mycoplasma	SOP-CH-320A	No contamination detected	Pass
Karyotype by G-banding	SOP-CH-003B	Normal karyotype	Pass

Electronic versions of this certificate of analysis (CoA) complete with electronic copies of individual reports, results, and procedures are available on our website, www.wicell.org. There are also archived CoAs for past cell lots.

Cells distributed by the National Stem Cell Bank are intended for research purposes only and are not intended for use in humans. These cells have undergone testing and are not known to harbor pathogens. However, appropriate biosafety precautions should be followed when working with these cells. The end user is responsible for ensuring that the cells are handled and stored in an appropriate manner. The NSCB is not responsible for damages or injuries that may result from the use of these cells.

Please visit the technical service portion of the website for assistance with your human ES Cells. The knowledgeable technical support staff can assist with embryonic stem cell culture concerns, training, and any other customer service concerns you may encounter.

Amendment(s):

Reason for Amendment	
CoA updated to include copyright information and electronic signature. Links updated.	
Original CoA	26-June-2008

Date of Lot Release	Quality Assurance Approval
06-June-2008	12/30/2013 X AMC AMC Quality Assurance Signed by:



Short Tandem Repeat Analysis*

Sample Report: 0183-STR

UW HLA#: 58829

Sample Date: 06/05/08

Received Date: 06/06/08

Requestor: WiCell Research Institute

Test Date: 06/06/08

File Name: 080606

Report Date: 06/11/08

Sample Name: (label on tube)

0183-STR

Description: DNA Extracted by WiCell

194 ug/mL; 260/280 = 1.92

Locus	Repeat #	STR Genotype
D16S539	5, 8-15	11,12
D7S820	6-14	9,13
D13S317	7-15	11,11
D5S818	7-15	10,12
CSF1PO	6-15	10,11
TPOX	6-13	8,9
Amelogenin	NA	X,Y
TH01	5-11	6,8
vWA	11, 13-21	17,19

Comments: Based on the 0183-STR DNA dated 06/05/08 and received on 06/06/08 from WI Cell, this sample (UW HLA# 58829) matches exactly the STR profile of the human stem cell line ES05 comprising 15 allelic polymorphisms across the 8 STR loci analyzed. No STR polymorphisms other than those corresponding to the human ES05 stem cell line were detected and the concentration of DNA required to achieve an acceptable STR genotype (signal/noise) was equivalent to that required for the standard procedure (~1 ng/amplification reaction) from human genomic DNA. These results suggest that the 0183-STR DNA sample submitted corresponds to the ES05 stem cell line and it was not contaminated with any other human stem cells or a significant amount of mouse feeder layer cells. Sensitivity limits for detection of STR polymorphisms unique to either this or other human stem cell lines is ~5%. A preliminary copy of this report was issued via electronic mail to the Cytogenetics department and Jeff Jones of WI Cell Research Institute on Thursday, June 12, 2008.



HLA/Molecular Diagnostics Laboratory



HLA/Molecular Diagnostics Laboratory



^{*} Testing to assess engraftment following bone marrow transplantation was accomplished by analysis of human genetic polymorphisms at STR loci. This methodology has not yet been approved by the FDA and is for investigational use only.

File: Final STR Report




This report is confidential. No part may be used for advertising or public announcement without written permission. Results apply only to the sample(s) tested.



Report Number 772956 Page 5 of 5

April 17, 2008 P.O. #:



STERILITY TEST REPORT

Sample Information:

4: ES05-FTDL-1, hES cells (ESO5-FTDL-1 P36MW)

Date Received:

April 01, 2008 April 02, 2008

Date in Test:
Date Completed:

April 16, 2008

Test Information:

Test Codes: 30744, 30744A

Immersion, USP / 21 CFR 610.12 Procedure #: BS210WCR.02

TEST PARAMETERS	PRODUCT				
Approximate Volume Tested	0.5 mL	0.5 mL 2			
Number Tested	2				
Type of Media	SCD	FTM 400 mL			
Media Volume	400 mL				
Incubation Period	14 Days	14 Days			
Incubation Temperature	20 °C to 25 °C	30 °C to 35 °C			
RESULTS	2 NEGATIVE	2 NEGATIVE			

	(4)	Page 1 Signed		Page 1 Signed
QA Reviewed:			Reviewed:	





FINAL STUDY REPORT

STUDY TITLE:

MYCOPLASMA DETECTION:

"Points to Consider"

PROTOCOL NUMBER:

30055E

TEST ARTICLE IDENTIFICATION:

ES05-FTDL-1

SPONSOR:

PERFORMING LABORATORY:

WuXi AppTec, Inc.



STUDY NUMBER:

106276

RESULT SUMMARY:

Considered negative for mycoplasma

contamination

Reference PO #



WiCell Research Institute

Page 2 of 9



Copy of Original

QUALITY ASSURANCE UNIT SUMMARY

STUDY: Mycoplasma Detection: "Points to Consider"

The objective of the Quality Assurance Unit is to monitor the conduct and reporting of nonclinical laboratory studies. This study has been performed under Good Laboratory Practices regulations (FDA, 21 CFR, Part 58 - Good Laboratory Practice for Nonclinical Laboratory Studies) and in accordance to standard operating procedures and a standard protocol. The Quality Assurance Unit maintains copies of study protocols and standard operating procedures and has inspected this study on the dates listed below. Studies are inspected at time intervals to assure the quality and integrity of the study.

 Critical Phase
 Date
 Study Director
 Management

 Staining of Coverslips
 05/19/08
 05/19/08
 06/18/08

 Final Report
 06/17/08
 06/17/08
 06/18/08

The findings of these inspections have been reported to management and the Study Director

Quality Assurance Auditor:_

Date: 06/18/2008.

GOOD LABORATORY PRACTICES STATEMENT

The study referenced in this report was conducted in compliance with U.S. Food and Drug Administration Good Laboratory Practice (GLP) regulations set forth in 21 CFR part 58

The studies not performed by or under the direction of WuXi AppTec, Inc , are exempt from this Good Laboratory Practice Statement and include characterization and stability of the test compound(s)/test article

Study Director:		Date:_	6018108	
, _				

Professional Personnel Involved:



Vice President of St Paul Operations Manager, Mycoplasma Testing Laboratory Study Director Client Relations Manager

WiCell Research Institute

Page 3 of 9



Copy of Original

1.0 PURPOSE

To demonstrate that a test article consisting of a cell bank, production or seed lots, or raw materials is free of mycoplasmal contamination, according to "Points to Consider" criteria

2.0 SPONSOR:

WiCell Research Institute

3.0 TEST FACILITY:

WuXi AppTec, Inc

4.0 SCHEDULING

DATE SAMPLE RECEIVED:

05/13/08

STUDY INITIATION DATE:

05/14/08

STUDY COMPLETION DATE:

06/18/08

5.0 TEST ARTICLE IDENTIFICATION: WiCell Research Institute; ES05-FTDL-1

6.0 SAMPLE STORAGE

Upon receipt by the Sample Receiving Department, the test samples were placed in a designated, controlled access storage area ensuring proper temperature conditions. Test and control article storage areas are designed to preclude the possibility of mix-ups, contamination, deterioration or damage. The samples remained in the storage area until retrieved by the technician for sample preparation and/or testing. Unused test samples remained in the storage area until the study was completed. Once completed, the remaining samples were discarded or returned as requested by the Sponsor

7.0 TEST ARTICLE CHARACTERIZATION

The Sponsor was responsible for all test article characterization data as specified in the GLP regulations. The identity, strength, stability, purity, and chemical composition of the test article were solely the responsibility of the Sponsor. The Sponsor was responsible for supplying to the testing laboratory results of these determinations and any others that may have directly impacted the testing performed by the testing laboratory, prior to initiation of testing. Furthermore, it was the responsibility of the Sponsor to ensure that the test article submitted for testing was representative of the final product that was subjected to materials characterization. Any special requirements for handling or storage were arranged in advance of receipt and the test article was received in good condition.

The Vero cells were maintained by WuXi AppTec's Cell Production Laboratory

8.0 EXPERIMENTAL DESIGN

8.1 Overview

Whereas no single test is capable of detecting all mycoplasmal strains, freedom from mycoplasmal contamination may be demonstrated by the use of both an indirect and direct procedure.

WiCell Research Institute

Page 4 of 9



Copy of Original

8.2 Justification for Selection of the Test System

Contamination of cell cultures by mycoplasma is a common occurrence and is capable of altering normal cell structure and function. Among other things, mycoplasma may affect cell antigenicity, interfere with virus replication, and mimic viral actions. Testing for the presence of mycoplasma for cell lines used to produce biologicals is recommended by the FDA, Center for Biologics Evaluation and Research (CBER) under "Points to Consider"

9.0 EXPERIMENTAL SUMMARY

The indirect method of detection allows visualization of mycoplasma, particularly non-cultivable strains, by growing the mycoplasma on an indicator cell line and then staining using a DNA-binding fluorochrome stain. The indicator cell line should be easy to grow, have a large cytoplasmic to nuclear area ratio and support the growth of a broad spectrum of mycoplasma species. The African green monkey kidney cell line, Vero, fits this description and was used in this assay. The assay was performed with negative and positive controls. Both a strongly cyto-adsorbing (*M. hyorhinis*) and a poorly cyto-adsorbing (*M. orale*) mycoplasma species were used as positive controls. Poor cyto-adsorbing mycoplasma species may not give reliable positive results when inoculated in low numbers. A second dilution of *M. orale* was used to ensure cyto-adsorption. Staining the cultures with DNA binding fluorochrome allows for the detection of mycoplasma based on the staining pattern observed. Only the cell nuclei demonstrate fluorescence in the negative cultures but nuclear and extra-nuclear fluorescence is observed in positive cultures.

Direct cultivation is a sensitive and specific method for the detection of mycoplasma. The agar and broth media employed supply nutrients necessary for the growth of cultivable mycoplasmas. These media also supply a source of carbon and energy, and favorable growth conditions. The direct assay was performed with both negative and positive controls. A fermentative mycoplasma (*M. pneumoniae*) and a non-fermentative mycoplasma (*M. orale*) were used as positive controls. The procedure employed in this study is based on the protocol described in the 1993 Attachment # 2 to the "Points To Consider" document, as recommended by the FDA, Center for Biologics Evaluation and Research (CBER)

10.0 TEST MATERIAL PREPARATION

10.1 Test Article Identification:

Test Article Name: General Description:

hES cells 1 x 40 mL

ES05-FTDL-1

Number of Aliquots used: Stability (Expiration): Storage Conditions:

Not Applicable
Ultracold (< -60°C)

Safety Precautions:

BSL-1

10.2 Test Sample Preparation

The test article was thawed in a water bath at $37 \pm 2^{\circ}\text{C}$ and 1:5 and 1:10 dilutions of the test article were prepared in sterile phosphate buffered saline (PBS). 1.0 mL of the undiluted sample, the 1:5 and 1:10 dilutions were then inoculated onto each of two (2) coverslips (per sample/dilution) containing Vero cells. The coverslips were incubated in incubator E770 for 1-2 hours at $37 \pm 1^{\circ}\text{C}$ / $5 \pm 2^{\circ}\text{CO}_2$ and then 2.0 mL of EMEM, 8% Fetal Bovine Serum (FBS) was added to each coverslip. The coverslips were returned to incubator E770 at $37 \pm 1^{\circ}\text{C}$ / $5 \pm 2^{\circ}\text{CO}_2$. After three days of incubation, the coverslips were fixed, stained, and then read using an epifluorescent microscope.

WiCell Research Institute
Page 5 of 9



Copy of Original

0.2 mL of the undiluted test article was then inoculated onto each of two SP-4 agar plates, and 10 0 mL was inoculated into a 75 cm 2 flask containing 50 mL of SP-4 broth. The plates were placed in an anaerobic GasPak system and incubated at 36 \pm 1°C for a minimum of 14 days.

The broth flask was incubated aerobically at $36 \pm 1^{\circ}$ C, and subcultured onto each of two SP-4 agar plates (0.2 mL/plate) on Days 3, 7, and 14 These subculture plates were placed in an anaerobic GasPak system and incubated at $36 \pm 1^{\circ}$ C for a minimum of 14 days. The broth flask was read each working day for 14 days. The SP-4 agar plates (Day 0) were read after 14 days of incubation. The SP-4 broth subculture plates (Days 3, 7, and 14) were read after 14 days incubation.

10.3 Controls and Reference Materials

10.3.1 Sterile SP-4 broth served as the negative control for both the direct and indirect assays.

10.3.2 Positive Controls

a. Indirect Assay

- a.1 Strongly cyto-adsorbing species *M hyorhinis* GDL (ATCC #23839) at 100 or fewer colony forming units (CFU) per inoculum.
- **a.2** Poorly cyto-adsorbing species *M. orale* (ATCC #23714) at 100 or fewer CFU and at approximately 100 ID₅₀ per inoculum

b. Direct Assay

- **b.1** Nonfermentative mycoplasma species *M* orale (ATCC #23714) at 100 or fewer CFU per inoculum
- **b.2** Fermentative mycoplasma species *M* pneumoniae FH (ATCC #15531) at 100 or fewer CFU per inoculum.

10,3,3 Control Preparation

a. Negative Controls

- a.1 1.0 mL of sterile SP-4 broth was inoculated onto each of two
 (2) coverslips containing Vero cells to serve as the negative control in the indirect assay
- a.2 0.2 mL of SP-4 broth was inoculated onto each of two (2) SP-4 agar plates to serve as the negative control in the direct assay. 10.0 mL of SP-4 broth was inoculated into a 75 cm² flask containing 50 mL of SP-4 broth to serve as the negative control in the direct assay.

WiCell Research Institute Page 6 of 9



Copy of Original

b. Positive Controls

- b.1 *M hyorhinis, M. orale,* and *M pneumoniae* were diluted to less than 100 CFU per inoculum in sterile SP-4 broth 1.0 mL of *M hyorhinis* and *M orale* at less than 100 CFU/mL was inoculated onto each of two (2) coverslips containing Vero cells 10 mL of *M orale* at 100 ID₅₀ CFU per inoculum was also inoculated onto each of two (2) coverslips containing Vero cells These coverslips served as the positive controls in the indirect assay
- b.2 The coverslips were incubated in incubator E770 for 1-2 hours at $37 \pm 1^{\circ}\text{C}$ / $5 \pm 2\%$ CO₂ and then 2.0 mL of EMEM, 8% Fetal Bovine Serum (FBS) was added to each coverslip. The coverslips were returned to incubator E770 at $37 \pm 1^{\circ}\text{C}$ / $5 \pm 2\%$ CO₂. After three days of incubation, the cell cultures were fixed, stained, and then read using an epifluorescent microscope.
- b.3 0.2 mL of *M* orale and *M*. pneumoniae at less than 100 CFU/plate was inoculated onto each of two (2) SP-4 agar plates 10.0 mL of *M*. orale and *M* pneumoniae at less than 10 CFU/mL (≤100 CFU/inoculum) were each inoculated into a 75 cm² flask containing 50 mL of sterile SP-4 broth.
- b.4 The agar plates were placed in an anaerobic GasPak system and incubated at 36 ± 1°C for 14 days. The broth cultures were incubated aerobically at 36 ± 1°C for a minimum of 14 days and were read each working day for 14 days. On Days 3, 7, and 14, 0.2 mL from each broth culture flask was subcultured onto each of two (2) SP-4 agar plates. These subculture plates were placed in an anaerobic GasPak system and incubated at 36 ± 1°C. The subculture plates were observed microscopically for the presence of mycoplasma colonies after a minimum of 14 days incubation.
- **c.** See Section 15.0, Results, for the results of these controls

11.0 DATA ANALYSIS

The results of this study were based on visual observations, therefore, no data analysis was required.

12.0 STATISTICAL METHODS

The results of this study were qualitative, therefore, no statistical analysis was required.



Copy of Original

13.0 EVALUATION CRITERIA

Final evaluation of the validity of the assay and test article results was based upon the criteria listed below and scientific judgment.

13.1 Indirect Assay

DETECTION OF MYCOPLASMA CONTAMINATION BY INDIRECT ASSAY

Controls	MYCOPLASMA FLUORESCENCE OBSERVED (AT LEAST ONE COVERSLIP REQUIRED FOR THE EVALUATION)
Negative Control	-
M. hyorhinis	+
M. orale (≤100 CFU)	+/-*
M. orale (100 ID ₅₀)	+

^{*}Mycoplasma must be observed for at least one dilution of the poorly cyto-adsorbing mycoplasma species M orale

13.2 Direct Assay

DETECTION OF MYCOPLASMA CONTAMINATION BY DIRECT ASSAY

	Negative Control	M. PNEUMONIAE	M. ORALE
Broth (Color change or turbidity change)	-	+/-	+/-
Agar Day 0 (at least one plate)	-	+	+
Agar Day 3, 7, 14 (at least one plate on one day)	1	+	+
Results	-	+	+

14.0 TEST EVALUATION

14.1 Indirect Assay

Hoechst stain will bind to most DNA containing organisms and organelles present in the culture; this includes indicator cell nuclei, prokaryotes including mycoplasma and cell debris. The source of DNA is determined by the staining pattern. The indicator cell nuclei fluoresce brightly and are generally 10-20 μ m in diameter. Mycoplasma fluorescence is less intense, is extra-nuclear and typically appears as small round bodies approximately 0.3 μ m in diameter.

14.2 Direct Assav

Change in color or turbidity of broth culture can be an indicator of the presence of mycoplasma growth. Fermentative mycoplasma produce acid from the carbohydrates in the medium causing the pH of the medium to drop and the broth to turn yellow in color. Nonfermentative mycoplasma produce ammonia by arginine hydrolysis causing the pH to rise and the broth to turn red. In general, growth of mycoplasma can cause the broth to become turbid. These changes must be confirmed by agar plate subculture or DNA-staining since changes in the appearance of the broth culture can also be caused by the properties of the inoculum

Mycoplasma colonies grow down into the agar causing the center of the colony to appear opaque and the peripheral surface growth to appear translucent. These "fried-egg" colonies vary in size, 10-500 μ m, and can be readily observed unstained using a light microscope.

Page 8 of 9



Copy of Original

14.3 Indirect Assay and Direct Assay Results Interpretation

le:	71. 1. 7. 7. 7. 1. 1. 1. 1. 1. 1. 1. 1. 1. 1. 1. 1. 1.	Т	EST ARTIC	LE	
Mycoplasmal fluorescence	-	+	+/-	+/-	-
Broth (Color change or turbidity change)	-	+/-	+/-	+/-	+*
Agar - Day 0 (at least one plate)	_	+/-	+/-	+	-
Agar - Day 3, 7, 14 (at least one plate on one day)	-	+/-	+	+/-	-
THEN: OVERALL FINAL RESULT	-	+	+	+	-

^{*}A change in the appearance of a broth culture must be confirmed by positive subculture plate(s)

14.4 Positive Results

The test article is considered positive if the direct assay (agar or broth media procedure) or the indirect assay (indicator cell culture procedure) show evidence of mycoplasma contamination and resemble the positive controls for the procedure

14.5 Negative Results

The test article is considered as negative if both the direct assay (agar and broth media procedure) and the indirect assay (indicator cell culture procedure) show no evidence of mycoplasma contamination and resemble the negative control for each procedure.

15.0 RESULTS

Indirect Assay and Direct Assay Results

		ΈCΤ		
	INDIRECT	BROTH FLASKS	Agar Plates	OVERALL
Test Article: ES05-FTDL-1	Negative	Negative	Negative	Negative
Negative Control	Negative	Negative	Negative	Negative
M. hyorhinis	Positive			Positive
M. orale	Positive	Positive	Positive	Positive
M pneumoniae		Positive	Positive	Positive

For the indirect assay, the coverslips for the undiluted test article were read and determined negative.

16.0 ANALYSIS AND CONCLUSION

- 16.1 The results of the negative and positive controls indicated the validity of this test.
- 16.2 These findings indicated that the test article, ES05-FTDL-1, is considered negative for the presence of mycoplasma contamination.

WiCell Research Institute
Page 9 of 9



Copy of Original

17.0 DEVIATIONS: None.

18.0 AMENDMENT #1: The study directorship was reassigned to Sheri Zielinski.

19.0 RECORD RETENTION

An exact copy of the original final report and all raw data pertinent to this study will be stored at WuXi AppTec, Inc., 2540 Executive Drive, St. Paul, MN 55120. It is the responsibility of the Sponsor to retain a sample of the test article

20.0 TECHNICAL REFERENCES

- 20.1 Barile, Michael F and McGarrity, Gerard J. (1983). "Isolation of Mycoplasmas from Cell Culture by Agar and Broth Techniques." Methods in Mycoplasmology, Vol II, ed J.G. Tully and S. Razin. (New York: Academic Press) pp. 159-165.
- 20.2 Del Giudice, Richard A and Joseph G. Tully 1996 "Isolation of Mycoplasma from Cell Cultures by Axenic Cultivation Techniques," ed J G Tully and S Razin, Molecular and Diagnostic Procedures in Mycoplasmology, Vol II (New York: Academic Press)
- 20.3 McGarrity, Gerard J. and Barile, Michael F. 1983 "Use of Indicator Cell Lines for Recovery and Identification of Cell Culture Mycoplasmas," ed J.G. Tully and S. Razin, Methods in Mycoplasmology, Vol. II (New York: Academic Press)
- 20.4 Masover, Gerald and Frances Becker 1996 "Detection of Mycoplasma by DNA Staining and Fluorescent Antibody Methodology," ed. J G Tully and S Razin, Molecular and Diagnostic Procedures in Mycoplasmology, Vol. II (New York: Academic Press)
- 20.5 Schmidt, Nathalie J and Emmons, Richard W 1989. "Cell Culture Procedures for Diagnostic Virology," ed Nathalie J Schmidt and Richard W Emmons, 6th ed, Diagnostic Procedures for Viral, Rickettsial and Chlamydial Infections (Washington: American Public Health Association).
- 20.6 U.S. Food and Drug Administration (FDA) Center for Biologics Evaluation and Research (CBER). 1993 "Points to Consider in the Characterization of Cell Lines Used to Produce Biologicals."

(For Laboratory Use Only)

AppTec Study # (')(',) \(\frac{1}{2} \) (c

Copy of Original

PROTOCOL TITLE:

MYCOPLASMA DETECTION: "POINTS TO CONSIDER"

TEST CODE:

30055

PERFORMING LABORATORY:

AppTec Laboratory Services

EFFECTIVE DATE:

11 December 2006

GLP PROTOCOL:

30055E



Technical Management

Quality Assurance has reviewed this protocol for compliance with applicable regulatory requirements and internal procedures

PROPRIETARY INFORMATION

THIS DOCUMENT IS THE PROPERTY OF AND CONTAINS PROPRIETARY INFORMATION OF APPTEC LABORATORY SERVICES. NEITHER THIS DOCUMENT NOR INFORMATION CONTAINED HEREIN IS TO BE REPRODUCED OR DISCLOSED TO OTHERS, IN WHOLE OR IN PART, NOR USED FOR ANY PURPOSE OTHER THAN THE PERFORMANCE OF THIS WORK ON BEHALF OF THE SPONSOR. WITHOUT PRIOR WRITTEN PERMISSION OF APPTEC LABORATORY SERVICES.

Protocol Number: 30055E

Effective Date: 11 December 2006

Page 2 of 8

Copy of Original

MYCOPLASMA DETECTION: "POINTS TO CONSIDER"

1.0 PURPOSE

This test is designed to demonstrate that a test article consisting of a cell bank, production or seed lots, or raw materials is free of mycoplasmal contamination, according to "Points to Consider" criteria.

2.0 TEST FACILITY: AppTec

AppTec Laboratory Services

3.0 SCHEDULING / DISCLAIMER

- 3.1 Test protocol initiation is generally within 10 working days after receipt of the test article and a signed protocol or request form. The Sample Submission Form serves as an addendum to this protocol. Written notification of the proposed initiation and completion dates will be provided at the time the test article and signed protocol are received by the laboratory. The estimated testing time is 28 days. Verbal results will be available from the Study Director upon completion of the study with the written quality assurance audited report to follow approximately 10 working days after completion of the study.
- 3.2 If a test, or a portion of it, must be repeated due to failure by AppTec to adhere to specified procedures, it will be repeated free of charge. If a test must be repeated, or a portion of it, due to failure of internal controls or failure to meet assay validity requirements, it will be repeated free of charge. "Methods Development" fees shall be assessed, however, if the test article and test system require modifications due to complexity and difficulty of testing.
- 3.3 If the Sponsor requests a repeat test, they will be charged for an additional test.
- 3.4 Neither the name of AppTec nor any of its employees are to be used in advertising or other promotion without written consent from AppTec
- 3.5 The Sponsor is responsible for any rejection of the final report by the regulatory agency concerning report format, pagination, etc. To prevent rejection, the Sponsor should carefully review the AppTec final report and notify AppTec of any perceived deficiencies in these areas before submission of the report to the regulatory agency. AppTec will make reasonable changes deemed necessary by the Sponsor, without altering the technical data.

4.0 TEST ARTICLE IDENTIFICATION

Test article information to be included in the final report will be provided solely by the Sponsor on the AppTec Sample Submission Form attached to this protocol.

5.0 TEST ARTICLE CHARACTERIZATION

The Sponsor is responsible for all test and control article characterization data as specified in the GLP regulations. The identity, strength, stability, purity, and chemical composition of the test article is solely the responsibility of the Sponsor. The Sponsor is responsible for supplying to the testing laboratory results of these determinations and any others that may directly impact the testing performed by the testing laboratory, prior to initiation of testing. Furthermore, it is the responsibility of the Sponsor to ensure that the test article submitted for testing is representative of the final product that will be subjected to materials characterization. Any special requirements for handling or storage must be arranged in advance of receipt and the test article must be received in good condition.

Protocol Number: 30055E Effective Date: 11 December 2006

Page 3 of 8

Copy of Original

The test article will be maintained according to the Sponsor's instructions
The VERO cells are maintained by AppTec's Cell Production Laboratory

6.0 EXPERIMENTAL DESIGN

6.1 Overview

Whereas no single test is capable of detecting all mycoplasmal strains, freedom from mycoplasmal contamination may be demonstrated by the use of both an indirect and a direct procedure

The indirect method of detection allows visualization of mycoplasma, particularly non-cultivable strains, by growing the mycoplasma on an indicator cell line and then staining using a DNA-binding fluorochrome stain (Hoechst stain). The indicator cell line should be easy to grow, have a large cytoplasmic to nuclear area ratio and support the growth of a broad spectrum of mycoplasma species. The African green monkey kidney cell line, VERO, fits this description and is frequently used.

The assay is performed with negative and positive controls. Both a strong cyto-adsorbing (*M hyorhinis*) and a poor cyto-adsorbing (*M orale*) mycoplasma species are used as positive controls. Poor cyto-adsorbing mycoplasma species may not give reliable positive results when inoculated in low numbers. A second dilution of *M orale* may be used to ensure cyto-adsorption. Staining the cultures with DNA-binding fluorochrome allows for the detection of mycoplasma based on the staining pattern observed. Only the cell nuclei demonstrate fluorescence in the negative cultures but nuclear and extra-nuclear fluorescence is observed in positive cultures.

Direct cultivation is a sensitive and specific method for the detection of mycoplasma. The agar and broth media employed supply nutrients necessary for the growth of cultivable mycoplasmas. These media also supply a source of carbon and energy, and favorable growth conditions. The procedure employed in this study is based on the methods described in the 1993 Attachment # 2 to the "Points To Consider" document.

6.2 Justification For Selection Of The Test System

Contamination of cell cultures by mycoplasma is a common occurrence and is capable of altering normal cell structure and function. Among other things, mycoplasma may affect cell antigenicity, interfere with virus replication and mimic viral actions. Testing for the presence of mycoplasma for cell lines used to produce biologicals is recommended by the FDA, Center for Biologics Evaluation and Research (CBER) under Points to Consider

7.0 PROCEDURE FOR IDENTIFICATION OF THE TEST SYSTEM

7.1 Controls And Reference Materials

- **7.1.1** Sterile SP-4 glucose broth will serve as the negative control inoculum for the direct and indirect assays
- **7.1.2** Optional: Cell culture medium may be added as an additional negative control for the indirect assay.

Effective Date: 11 December 2006

Page 4 of 8

Copy of Original

7.1.3 Positive Controls

a. Indirect Assay

- a.1 Strongly cyto-adsorbing species M. hyorhinis GDL (ATCC #23839) at 100 or fewer colony forming units (CFU) per inoculum.
- a.2 Poorly cyto-adsorbing species *M orale* (ATCC #23714) at 100 or fewer CFU and at approximately 100 ID₅₀ per inoculum

b. Direct Assay

- b.1 Nonfermentative mycoplasma species *M orale* (ATCC#23714) at 100 or fewer CFU per inoculum
- **b.2** Fermentative mycoplasma species *M pneumoniae* FH (ATCC #15531) at 100 or fewer CFU per inoculum
- 7.2 Testing is performed in strict adherence to AppTec Standard Operating Procedures (SOPs) which have been constructed to cover all aspects of the work including, but not limited to, receipt, identification, log-in, and tracking of test article(s). Additionally, each test is assigned a unique Project Number. This number is used for identification during the course of the test.

8.0 TEST METHOD

Protocol Number: 30055E

8.1 Indirect (DNA-staining) Assay

- 8.1.1 Inoculate no less than 1.0 mL of the negative control and test article directly onto coverslips containing previously incubated VERO cells. Two (2) or more coverslips will be used for each control and test article. Additional dilutions of the test article may be made to eliminate interference of cellular debris with mycoplasma detection.
- 8.1.2 For media samples (EMEM, DMEM, FBS, etc.) that are free of cellular material, inoculate 1.0 mL of undiluted test article onto four (4) coverslips containing previously incubated VERO cells. Three (3) coverslips will be observed and the fourth will serve as a backup
- 8.1.3 For trypsin samples, add an equal volume of previously tested and released fetal bovine serum (FBS) to inactivate the trypsin. 1.0 mL of undiluted test article will be inoculated onto four (4) coverslips containing previously incubated VERO cells. Three (3) coverslips will be observed and the fourth will serve as a backup.
- **8.1.4** The positive controls, *M hyorhinis* and *M orale*, are inoculated in the same manner, using 100 or fewer CFU per inoculum for *M hyorhinis* and 100 or fewer CFU and at approximately 100 ID₅₀ per inoculum for *M orale*.
- **8.1.5** Following reincubation for 3 to 5 days, cells are fixed with a DNA-binding fluorochrome (Hoechst 33258 stain), and are evaluated for the presence of mycoplasma using epifluorescent microscopy.

8.2 Direct (Microbiological) Assay

- **8.2.1** At least two (2) SP-4 glucose agar plates are inoculated with no less than 0.2 mL per plate of the negative control (sterile SP-4 glucose broth).
- 8.2.2 50 mL of sterile SP-4 glucose broth is inoculated with no less than 10 mL of the negative control.
- 8.2.3 The test article is then inoculated onto two (2) or more SP-4 glucose agar plates (0.2 mL per plate) and into one (1) broth flask (no less than 10 mL into 50 mL of sterile SP-4 glucose broth)
- 8.2.4 The positive controls, *M. pneumoniae* and *M. orale*, are inoculated in the same manner, using 100 or fewer CFU per inoculum onto each of two (2) or more plates and 10 mL (100 or less CFU per inoculum) into 50 mL of sterile SP-4 glucose broth.
- **8.2.5** Agar plates are incubated anaerobically in a GasPak system at 36 \pm 1°C for at least 14 days
- **8.2.6** Broth culture flasks are incubated aerobically at 36 ± 1 °C. Broth cultures are observed daily (normal working days only) for changes in color or turbidity.
- **8.2.7** The broth culture flasks are subcultured on Days 3, 7, and 14 onto SP-4 agar plates. Two (2) or more plates (0.2 mL broth / plate) are inoculated and incubated anaerobically in a GasPak system for at least 14 days.
- **8.2.8** The agar plates are examined microscopically for the presence of mycoplasma colonies after 14 or more days of incubation.
- 9.0 METHOD FOR CONTROL OF BIAS: Not applicable.

10.0 DATA ANALYSIS

The results of this study are based on visual observations; therefore no data analysis is required.

11.0 STATISTICAL METHODS

The results of this study are qualitative; therefore no statistical analysis is required.

12.0 ASSAY VALIDITY

Final evaluation of the validity of the assay and test article results will be based upon the criteria listed below and scientific judgment.

12.1 Indirect Assay

DETECTION OF MYCOPLASMA CONTAMINATION BY INDIRECT ASSAY

CONTROLS	MYCOPLASMA FLUORESCENCE OBSERVED (AT LEAST ONE COVERSLIP REQUIRED FOR THE EVALUATION)
Negative Control	-
M. hyorhinis	+
M. orale (≤100 CFU)	+/-*
M. orale (100 ID ₅₀)	+

^{*}Mycoplasma must be observed for at least one dilution of the poorly cytoadsorbing mycoplasma species M. orale

Page 6 of 8

12.2 Direct Assav

DETECTION OF MYCOPLASMA CONTAMINATION BY DIRECT ASSAY

	NEGATIVE CONTROL	M. PNEUMONIAE	M. ORALE
Broth (Color change or turbidity change)	-	+/-	+/-
Agar Day 0 (at least one plate)	_	+	+
Agar Day 3, 7, 14 (at least one plate on one day)	-	+	+
Results	-	+	+

13.0 TEST EVALUATION

13.1 Indirect Assay

Hoechst stain will bind to most DNA containing organisms and organelles present in the culture; this includes indicator cell nuclei, prokaryotes including mycoplasma and cell debris. The source of DNA is determined by the staining pattern. The indicator cell nuclei fluoresce brightly and are generally 10 to 20 μ m in diameter. Mycoplasma fluorescence is less intense, is extra-nuclear and typically appears as small round bodies approximately 0.3 μ m in diameter.

13.2 Direct Assay

Change in color or turbidity of broth culture can be an indicator of the presence of mycoplasma growth. Fermentative mycoplasma produce acid from the carbohydrates in the medium causing the pH of the medium to drop and the broth to turn yellow in color. Nonfermentative mycoplasma produce ammonia by arginine hydrolysis causing the pH to rise and the broth to turn red. In general, growth of mycoplasma can cause the broth to become turbid. These changes must be confirmed by agar plate subculture or DNA-staining since broth changes can also be caused by the properties of the inoculum.

Mycoplasma colonies grow down into the agar causing the center of the colony to appear opaque and the peripheral surface growth to appear translucent. These "fried-egg" colonies vary in size, 10-500 μm , and can be readily observed unstained using a light microscope

13.3 Indirect Assay and Direct Assay Results Interpretation

ip:	10111111111	TE	ST ART	ICLE	
Mycoplasmal fluorescence	-	+	+/-	+/-	-
Broth (Color change or turbidity change)	_	+/-	+/-	+/-	+*
Agar - Day 0 (at least one plate)	-	+/-	+/-	+	-
Agar - Day 3, 7, 14 (at least one plate on one day)	-	+/-	+	+/-	-
THEN: OVERALL FINAL RESULT	-	+	+	+	-

^{*}A change in the appearance of the broth culture must be confirmed by positive subculture plate(s)

Page 7 of 8

13.4 **Negative Results**

Protocol Number: 30055E

The test article is considered as negative if both the direct assay (agar and broth media procedure) and the indirect assay (indicator cell culture procedure) show no evidence of mycoplasma contamination and resemble the negative control for each procedure.

13.5 Positive Results

The test article is considered positive if the direct assay (agar and/or broth media procedure) or the indirect assay (indicator cell culture procedure) show evidence of mycoplasma contamination and resemble the positive controls for each procedure

13.6 Repeat Assavs

A test will be repeated in part or in total if a control failure occurs.

14.0 PROTOCOL CHANGES

If it becomes necessary to make changes in the approved protocol, the revisions and reasons for changes will be documented, signed by the Study Director, dated, maintained with the protocol and reported to the Sponsor. If an event occurs which may have an effect on the validity of the study, the Sponsor will be notified as soon as is practical. If the Study Director is unable to complete the study, an alternate Study Director with full responsibility and authority regarding the study will be assigned.

15.0 **FINAL REPORT**

The final report will include but will not be limited to: the date of the study initiation and completion, the purpose as stated in the approved protocol, changes in the approved protocol, identification of the test system, a description of the methods used and conclusion as it relates to the test.

16.0 RECORD RETENTION

16.1 **Study Specific Documents**

All of the original raw data developed exclusively for this study shall be retained according to AppTec Laboratory Services' standard operating procedures for archival. These original data include, but are not limited to the following:

- 16.1.1 All handwritten and equipment generated raw data for control(s) and test article(s).
- **16.1.2** Any protocol amendments/deviation notifications
- 16.1.3 Memoranda, specifications, and other study specific correspondence relating to interpretation and evaluation of data, other than those documents contained in the final study report
- 16.1.4 Original signed protocol.
- **16.1.5** Certified copy of final study report.
- 16.1.6 Study-specific SOP deviations made during the study

16.2 **Facility Specific Documents**

The following records shall also be retained according to AppTec Laboratory Services' standard operating procedures for archival. These documents include, but are not limited to, the following:

- 16.2.1 SOPs which pertain to the study conducted.
- 16.2.2 Non study-specific SOP deviations made during the course of this study which may affect the results obtained during this study.
- 16.2.3 Methods which were used or referenced in the study conducted.

Effective Date: 11 December 2006

Page 8 of 8

Copy of Original

16.2.4 QA reports for each QA inspection with comments.

16.2.5 Facility Records: Temperature Logs (ambient, incubator, etc.), Instrument Logs, Calibration and Maintenance Records.

16.2.6 Current job descriptions and summary of experience and training for all personnel involved in the study.

17.0 REFERENCES

Protocol Number: 30055E

- Barile, Michael F and McGarrity, Gerard J. (1983) "Isolation of Mycoplasmas from Cell Culture by Agar and Broth Techniques." Methods in Mycoplasmology, Vol II, ed. J.G. Tully and S. Razin. (New York: Academic Press) pp. 159-165.
- Del Giudice, Richard A. and Tully, Joseph G. 1996. "Isolation of Mycoplasma from Cell Cultures by Axenic Cultivation Techniques," ed. J.G. Tully and S. Razin, Molecular and Diagnostic Procedures in Mycoplasmology, Vol. II (New York: Academic Press)
- 17.3 McGarrity, Gerard J. and Barile, Michael F. 1983. "Use of Indicator Cell Lines for Recovery and Identification of Cell Culture Mycoplasmas," ed. J.G. Tully and S Razin, Methods in Mycoplasmology, Vol. II (New York: Academic Press).
- 17.4 Masover, Gerald and Frances Becker. 1996. "Detection of Mycoplasma by DNA Staining and Fluorescent Antibody Methodology," ed. J.G. Tully and S. Razin, Molecular and Diagnostic Procedures in Mycoplasmology, Vol. II (New York: Academic Press).
- 17.5 Schmidt, Nathalie J. and Emmons, Richard W. 1989. "Cell Culture Procedures for Diagnostic Virology," ed. Nathalie J. Schmidt and Richard W. Emmons, 6th ed., Diagnostic Procedures for Viral, Rickettsial and Chlamydial Infections (Washington: American Public Health Association).
- 17.6 U.S Food and Drug Administration (FDA) Center for Biologics Evaluation and Research (CBER). 1993 "Points to Consider in the Characterization of Cell Lines Used to Produce Biologicals."

18.0 COMPLIANCE

GLP STATUS: This study will be performed in accordance with Good Laboratory Practices for Nonclinical Laboratory Studies as found in Title 21 Code of Federal Regulations Part 58

19.0 TEST ARTICLE DISPOSITION

It is the responsibility of the Sponsor to retain a sample of the test material. All unused test material will be discarded following study completion unless otherwise requested by Sponsor.

Copy of Original

CHENT	PROTOCOL	ADDDOVAL	
OFICIAL	TRU TUGUL	APPROVAL	JEORM.

PLEASE NOTE THAT TESTING CANNOT BE INITIATED UNTIL THIS FORM IS COMPLETED WITH AN AUTHORIZED SIGNATURE AND THE ORIGINAL IS RETURNED TO APPTEC.



SPONSOR:

Ms. Erika Mitchen WiCell Research Institute 614 Walnut Street; 13th Floor P O. Box 7365 Madison, WI 53705

4000252 / WCR01 Phone #: 608-441-8019 Facsimile: 808-441 8011 E-mail: erika@wicell org

Primary Approval Statement

I have read AppTec Laboratory Services' client protocol, 30055E · Mycoplasma Detection: "Points To Consider" I accept the test method described | understand that my approval will be valid until one or both of the following occur:

The protocol is revised and a new version letter is issued

The Primary Approver's position with the Sponsor company is terminated or quanges, whichever may occur first.

	i li
NAME:	TITLE: QA Manager
SIGNATURE	DATE: 2/15/0-7
Associate(s) Ap	proval Statement
The Primary Approver (above) has authorized the submitting samples for testing under this protocol or submission will be valid until one or more of the	following Associate(s) to accept the responsibility for Each associate understands that their authorization following has occurred:
The protocol has been revised and new years	
Any of the Associate's positions with the Spor	isor company are terminated or change, whichever
	ciate's authorization by sending a signed and dated
	uthorized to initiate testing of samples under this
do wish to have the following Associate(s	authorized to initiate testing of samples under this
Mare designed and the second and the	
	Name of Associate (please print)
PPTEC LABORATORY SERVICES:	

NAME:

SIGNATU



Biopharmaceutical / Biological Products SAMPLE SUBMISSION FORM Complete <u>all</u> applicable areas on both pages of this form and enclose in sample shipment. A separate completed form is required for each lot and/or type of sample.

of Original

106 276

CLIENT CONTACT INFORMATION	İ	PHONE			FA	iX		EMAIL
Contact for Final Report:				60	£			
(if applicable/needed):								
(ii application sedect).								
Company Name and Address:			1	Client Ac	count	t Number: 4000	252	
				AppTec (Duote	Number: V	204 04220	10
						-		
				Pulchase	· Ora	er Number:		
CAME E DENTIFICATION & INCOMA	ELON	If resubmitting sample		nrovide orio	rinal A	nnTac samnle Acc	ession #	
SAMPLE IDENTIFICATION & INFORMA Sample Designation for Final Report:		11 Tesupiniting sumpri				e (General Des		Material):
- Sample Designation for Timal Report.				.,, _		. (
TOAT ETN.	i			INT.		Cella	 -	
ESO5-FTDL	-			NO.	\mathcal{L}	ممري	,	
Commercial/Marketed Product? Species of Ort	igin: Stal	bility (Expiration Da	te): Bio	safety Le	vel:	Sample Matri	x or Buffe	r Components (if applicable):
□Yes ★ANO NUMA	n			1				
				<u> </u>				
SAMPLE SHIPMENT & STORAGE								
						<u> </u>	(eit	Ultracold (< -60°C)
••••• <u> </u>	Temperature							
Liquid Nitrogen (Available only in Philadel	phia)	NOTE: For virol	ogy testii	ng sample				nined by the Study Director.
NOTE: For small-quantity liquid samples, AppTec has found the use of cryogenic vials with internal	🛛 Do Not	Freeze/Thaw Sar	nple for	Reuse		n test complet Returned (Ad		-
thread closures an effective way to help prevent	☐ May Fre	eeze/Thaw						et # for shipping:
leaking that can result in loss of sample volume and possible sample contamination during shipping.		# of Times:		İ				
				Ť				
SAMPLE CHARACTERIZATION INFORM	ATION							
Sample characterization information such as st	rength homo	geneity purity an	d stabili	ty and ot	hers	that may direc	tly impact	the testing performed:
☐ IS ATTACHED to this sample submission	form	🗹 IS UNAVAILA	BLE.		IS C	ONSIDERED	PROPRIE	TARY INFORMATION
	,							
IF SUBMITTING A CELL LINE, COMPLE	TE THIS SE	CTION	NOTE:	Cells subi	mitte	d for expansion	will be sto	ored in liquid nitrogen.
Species and Cell Type:	Check On		ubcultui	ring: (Che	eck a	ppropriate box		
	☐ Suspe			ires Tryps				Cells are sensitive
	☐ Adher-	ent Cells 📗 🗌] Requ	ires Tryps	in/EI	O 🗆 ATC	her:	
Medium Requirements, Including Supplements/	Concentration	ns:					emperatu	re and % CO₂ for Growth:
NOTE: AppTec in-house medium and supplements will be u	unzed uniess sug	ррнеа ру снепт with sa	mpre			٠	C =	
						0	6 CO₂ =	
					10	alle Der Viel-		
FOR CRYOPRESERVED CELLS: See	eding Density				1 0	ells Per Vial:		
Cell Concentration / Conflic	ience Prior	Seeding Concer	ntration	OR		Number of D		Passage Level / Limit:
PASSAGE to Passage:		Split Ratio:				Between Pa	ssages:	
INFORMATION								

See Page 2 of this form to provide additional information and sample submission authorization

**X Stared at 2-60°C at William Apple: 51. Paul 5/14/08
Prepared Date: 11/26/07

REQUESTED TEST	TING If more space is	needed to list requested as	says, attach a se	cond copy of this sh	neet	
BRIEF NAME / DE	ESCRIPTION OF ASSAY	PROTOCOL NUMBER	For each protocol, indicate if		F MATERIAL ER PROTOCOL	Check if requestin STAT [Additiona
			R&D	# of Tubes Vol. In Tube I tube Vorticed 51(145)	fees apply	
lycoplasma		30055		1 tube		
				Verified		
				C 5/14	l ₂ 0	
					·	
					<u></u>	
	the state of the s					
			1			
	BROVIDE THE FOLLO	WING INFORMATION,	AS APPLICAB	1 F		
ordering Protocol # 37000, li	ist cell lines;			Check one:	LI Plates £	Flasks
oncentration per		For Patient o	or Test Dose	Check one:	□ 14-day □	I Flasks 28-day —
,	unit of measurement)			Check one:	□ 14-day □	
oncentration per (write in eneck One: Particles DR STERILITY TESTING:	unit of measurement)	DNA Detection Assays	Amount of ma	Check one:	□ 14-day - [28-day
oncentration per(write in a concentration per(write in a concentration per(write in a concentration per	unit of measurement) PFU For I Has this TYPE of sample been sui	DNA Detection Assays bmilted before? □Yes ample? □Yes □No	Amount of ma	Check one: Units: terial to test: sample contain a	□ 14-day □ □	28-day — — es □No
oncentration per	unit of measurement) For I Has this TYPE of sample been sult has B/F been conducted on this sample been the series of the sample been the series of the se	DNA Detection Assays bmitted before?	Amount of ma	Check one: Units: terial to test: sample contain a formation such as of	□ 14-day □ ntibiotics? □Ye	es 🗆 No
IMPORTANT INSTRUCTION Sample submission form—which must seemled that clients provide completionally to AppTec) Failure to provide in required because dittion if re-testing is required because metal that clients ground attach and additional fourly to AppTec) Failure to providition if re-testing is required because the control of the	unit of measurement) For I Has this TYPE of sample been suit Has B/F been conducted on this si EPARATION & SPECIAL INS CTIONS REGARDING THIS FOR it accompany each submitted sample – act le information on this form for ALL areas information that may be critical regarding ide this information could result in testin se of missing or incomplete information of the company of the critical regarding in the company of the critical regarding in the company of the critical regarding in t	bmitted before?	Amount of ma No Does Transfer BEFORE SIG Beta Being required in g, preparation etc.	Check one: Units: terial to test: sample contain a formation such as of the contain a formation cannot be (even if this information .	ntibiotics?	es No ution, etc.) icular sample spaces on this seen provided
IMPORTANT INSTRUCTION Seample submission form—which must client should attach any additional founds to the AppTech Faiture to provide complete fou	unit of measurement) For I Has this TYPE of sample been suit Has B/F been conducted on this si EPARATION & SPECIAL INS CTIONS REGARDING THIS FOR it accompany each submitted sample – act le information on this form for ALL areas information that may be critical regarding ide this information could result in testin se of missing or incomplete information of the company of the critical regarding in the company of the critical regarding in the company of the critical regarding in t	bmitted before?	Amount of ma No Does Transfer BEFORE SIG Beta Being required in g, preparation etc.	Check one: Units: terial to test: sample contain a formation such as of the contain a formation cannot be (even if this information .	ntibiotics?	es No ution, etc.) icular sample spaces on this seen provided

AppTec - Philadelphia - 4751 League Island Bivd - Philadelphia, PA 19112 - 800.622 8820 - 215.218 5500 - FAX 215.218 5990 AppTec - Atlanta - 1265 Kennestone Circle - Marietta, GA 30066 - 888.847.6633 - 770 514.0262 - FAX 770.514.0294 AppTec - St. Paul - 2540 Executive Drive - St. Paul - MN 55120 - 888.794 0077 - 651 675 2000 - FAX 651 675 2005



GLP COMPLIANT TEST PROTOCOL AMENDMENT

Copy of Original

20		1			
	Effective Date:	June 1	10, 2008		
3.0	Amendment Date:	June 1	10, 2008		
4.0	Sponsor:	WiCell Resear	ch Institute		
5.0	Test Facility:	WuXi AppTec	Inc		
60	WuXi AppTec Protoco	l Number:	30055E		
70	WuXi AppTec Project	Number:	106276		
80	Modification to Protoc The Study Directorship		as reassigned to She	i Zielinski.	
90	Reason for Change: Study director of	hange			
10.0	Impact to Protocol Inte	erpretation:			
11.0	Review Signatures below repre	sent authorizati	on of the amendmer	it (e.g. authorize change to the	SOP
	and protocol).				
Stu	and protocol).			UII3/08 Date NA	
				⊍।।3/০৪ Date	
Sponso	and protocol).	to protocol rotocol Vorksheet/Study		Date NA Date	

ALS-4508-3A

Page 1 of 1 Effective Date: 7/31/07



WiCell Cytogenetics Report: 000553-051308

NSCB 0183

Report Date: June 24, 2013

Case Details:

Cell Line: ES05-FTDL-1 (NSCB# 0183)

Passage #: NSCB 0183

Date Completed: 5/21/2008

Cell Line Gender: male

Investigator: National Stem Cell Bank

Specimen: hESC on MEF feeder

Date of Sample: 5/13/2008


Tests, Reason for: NSCB# 0183 - FTDL1 Testing

Results: 46,XY

Completed by CS, CLSp(CG), on 5/21/2008

Reviewed and interpreted by KDM, PhD, FACMG, on 5/21/2008

Interpretation: No abnormalities were detected at the stated band level of resolution.

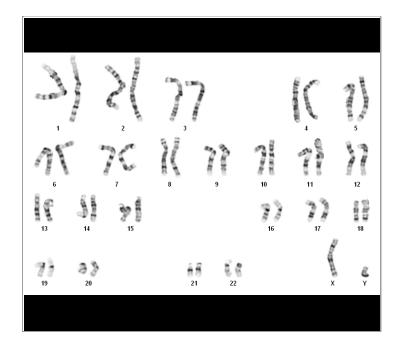

Cell: S01-04

Slide: B

Slide Type: Karyotyping

Cell Results: Karyotype: 46,XY

of Cells Counted: 20

of Cells Karyotyped: 4

of Cells Analyzed: 8

Band Level: 450-525

Results Transmitted by Fax / Email / Post Sent By:_____

Date:_____Sent To:_____