



Cell Line: WA01  
Lot: 10

**Table of Contents**

STR Report .....	2
Mycoplasma Report .....	3
Karyotype Report .....	8

This material predates when WiCell produced a certificate of analysis for each lot. Therefore, a certificate of analysis is not available. The following pages are the reports for the testing completed for this lot.

If you have any questions please contact WiCell's technical support staff via our website side at [www.wicell.org](http://www.wicell.org) and we will be happy to assist you.

Thank you,

WiCell

Short Tandem Repeat Analysis\*

Sample Report: H1p26 lot 10

UW HLA#: 55501

Sample Date: 12/26/06

Requestor: WICell Research Institute

Received Date: 01/02/07

Test Date: 01/09/07

File Name: 070110


Report Date: 01/11/07

Sample Name: (label on tube) H1 p26 lot 10

Description: Frozen pellet H1p26 lot 10 non-  
infectious hES cells with MEF feeder cells  
12/26/06 DF

Locus	Repeat #	STR Genotype
D16S539	5, 8-15	9,13
D7S820	6-14	8,12
D13S317	7-15	8,11
D5S818	7-15	9,11
CSFIPO	6-15	12,13
TPOX	6-13	8,11
Amelogenin	NA	X,Y
TH01	5-11	9.3,9.3
vWA	11, 13-21	15,17


Comments: The concentration of purified DNA isolated from the H1p26 Lot 10 human embryonic stem cell sample dated 12/26/06 and received 01/02/07 required to achieve an acceptable STR genotype (signal/noise) was equivalent to that required for the standard procedure (~1 ng/amplification reaction) from human genomic DNA.



1-16-07

Date

HLA/Molecular Diagnostics Laboratory



01/12/07

Date

HLA/Molecular Diagnostics Laboratory

\* Testing to assess engraftment following bone marrow transplantation was accomplished by analysis of human genetic polymorphisms at STR loci. This methodology has not yet been approved by the FDA and is for investigational use only.

File: Final STR Report



APPENDIX I

Document #: DCF3008A
Edition #: 06
Effective date: 9/17/2003
Title: DNA FLUOROCHROME ASSAY RESULTS

DNA-FLUOROCHROME ASSAY RESULTS
Procedures 3008, 3009, 3011

Sample ID # 46862 M-250 Date Rec'd: 12/13/2006 P.O. # [Redacted]

Indicator Cells Inoculated: Date/Initials: 12/14/06 / BMB

Fixation: Date/Initials: 12/18/06 / JA



Staining: Date/Initials: 12/18/06 / JA

TEST/CONTROL ARTICLE:

H1 p24

LOT# 10

Distribution
WiCell Research Institute



DNA FLUOROCHROME ASSAY RESULTS:

X NEGATIVE: A reaction with staining limited to the nuclear region, which indicates no mycoplasmal contamination.

POSITIVE: A significant amount of extranuclear staining which strongly suggests mycoplasmal contamination.

INCONCLUSIVE: A significant amount of extranuclear staining consistent with low - level mycoplasmal contamination or nuclear degeneration.

A significant amount of extranuclear staining consistent with bacterial, fungal or other microbial contaminant or viral CPE. Morphology not consistent for mycoplasmal contamination.

COMMENTS:

Date: 12/18/06 Results Read by: JA Date of Review: 12/18/06 Reviewed by: CM

Mycoplasma  
Testing ServicesBIONIQUE TESTING LABORATORIES, INC.  


## APPENDIX IIa

Document #: DCF9002B(assnt)

page 1 of 2

Edition #: gmp 04


Effective date: 9/17/2003

Title: QUALITY ASSURANCE REPORT - GMP

## QUALITY ASSURANCE REPORT - GMP

Catalog #: M-250Procedural Reference Numbers: 308, 301, 303Bionique Sample ID # 46862

This testing procedure was performed in compliance with Current Good Manufacturing Practice (cGMP) standards as specified under 21 CFR parts 210 and 211 to the extent to which these regulations pertain to the procedures performed. All records pertaining to the test/procedure have been reviewed by the Quality Assurance/Quality Control individual whose signature below verifies that the methods and procedures referenced above have been followed, and that the Final Report accurately reflects the raw data generated during the course of these procedures.

Date of full data review by Quality Assurance: 1/10/07Nicole M. Cook  
Quality Assistant, Bionique Testing Labs, Inc.1/10/07  
Date

All records, including raw data and final reports, are maintained by:

Quality Assurance  
Bionique Testing Laboratories, Inc.  
156 Fay Brook Drive  
Saranac Lake, NY 12983

Procedures specified in individual protocols are inspected at appropriate intervals according to a pre-determined schedule. Each lot of medium used for testing is examined for mycoplasmal growth-promoting properties, and must meet with required Quality Control performance criteria. Traceability of all of the components used in these protocols is assured, and documentation for individual lots will be supplied upon request.

## Additional Comments:

- I. The stability of the test and/or control sample material is the responsibility of the company submitting the sample prior to receipt at Bionique Testing Laboratories. Bionique Testing Laboratories will assume responsibility for sample stability following receipt and prior to being placed on test.
- II. This test is for the detection of microbiological growth and does not require statistical validation.

Document #: DCF9002B/assnt  
Edition #: gmp 04  
Effective date: 7/17/2003  
Title: QUALITY ASSURANCE REPORT - GMP

**REFERENCES:****REGULATORY:**

1. Title 21 CFR Part 210 - CURRENT GOOD MANUFACTURING PRACTICE IN MANUFACTURING, PROCESSING, PACKING, OR HOLDING OF DRUGS, GENERAL and 21 CFR Part 211 - CURRENT GOOD MANUFACTURING PRACTICE FOR FINISHED PHARMACEUTICALS. Federal Register, Food and Drug Administration.
2. Points to Consider in the Characterization of Cell Lines Used to Produce Biologicals (May, 1993); Director, Office of Biologics Research and Review, Food and Drug Administration.
3. Title 21 CFR PART 610.30 - General Biological Products Standards, Subpart D; Test for Mycoplasma. Federal Register, Food and Drug Administration.
4. Title 9 CFR PART 113.28 - Detection of Mycoplasma Contamination. Federal Register, Animal and Plant Health Inspection Service, United States Department of Agriculture

**GENERAL:**

5. Michael Barile and Jerome Kern. Isolation of *Mycoplasma arginini* from commercial bovine sera and its implication in contaminated cell cultures. *Proceedings of the Society for Experimental Biology and Medicine*, Volume 138, Number 2, November 1971.
6. Chen, T.R. *In situ* detection of mycoplasma contamination in cell cultures by fluorescent Hoechst 33258 stain. *Experimental Cell Research*, 104: 255-262, 1977.
7. A Guide to MYCOPLASMA DETECTION AND CONTROL. Bionique Testing Laboratories, Inc., 1992.
8. Carolyn K. Lincoln and Daniel J. Lundin. Mycoplasma Detection and Control. *U. S. Fed. for Culture Collections Newsletter*, Vol. 20, Number 4, 1990.
9. Fetal Bovine Serum; Proposed Guideline. National Committee For Clinical Laboratory Standards (NCCLS), Vol. 10, Number 6, 1990. (NCCLS publication M25-P).
10. Gerard J. McGarrity, Judi Sarama, and Veronica Vanaman. Cell Culture Techniques. *ASM News*, Vol. 51, No. 4, 1985.
11. J. G. Tully, S. Razin (eds.), *Methods in Mycoplasmaology*, Volumes I and II. Academic Press, N.Y., 1983.
12. M. F. Barile, S. Razin, J. G. Tully and R. F. Whitcomb (eds.), *The Mycoplasmas*, Volumes 1-4. Academic Press, N.Y., 1979.

Mycoplasma  
Testing Services



BIONIQUE TESTING LABORATORIES



APPENDIX IV

Document#: DCF3013D  
Edition#: 10  
Effective Date: 07/15/2003  
Title: M-250 FINAL REPORT SHEET

M-250 FINAL REPORT


Direct Specimen Culture  
Procedure 3008, 3011, 3013

TO: Distribution  
WiCell Research Institute



BTL SAMPLE ID#: 46862

P.O.#:



DATE REC'D: 12/13/2006

TEST/CONTROL ARTICLE:

H1 p24

LOT#: 10

DIRECT CULTURE SET-UP (DAY 0)

DATE: 12/13/2006

INDICATOR CELL LINE (VERO)

SEE DNA FLUOROCHROME RECORD SHEET

			DATE
THIOGLYCOLLATE BROTH	DAY 7	+ ⊖	<u>12/20/2006</u>
	DAY 28	+ ⊖	<u>01/10/2007</u>
BROTH-FORTIFIED COMMERCIAL <u>0.5</u> mL SAMPLE	DAY 7	+ ⊖	<u>12/20/2006</u>
	DAY 28	+ ⊖	<u>01/10/2007</u>
<u>6.0</u> mL BROTH	DAY 7	+ ⊖	<u>12/20/2006</u>
	DAY 28	+ ⊖	<u>01/10/2007</u>
BROTH-MODIFIED HAYFLICK <u>0.5</u> mL SAMPLE	DAY 7	+ ⊖	<u>12/20/2006</u>
	DAY 28	+ ⊖	<u>01/10/2007</u>
<u>6.0</u> mL BROTH	DAY 7	+ ⊖	<u>12/20/2006</u>
	DAY 28	+ ⊖	<u>01/10/2007</u>
BROTH-HEART INFUSION <u>0.5</u> mL SAMPLE	DAY 7	+ ⊖	<u>12/20/2006</u>
	DAY 28	+ ⊖	<u>01/10/2007</u>

(See Reverse)


APPENDIX IV

Document#: DCF3013D  
 Edition#: 10  
 Effective Date: 07/15/2003  
 Title: M-250 FINAL REPORT SHEET

SAMPLE ID#:	46862	AEROBIC	MICROAEROPHILIC	DATE
AGAR PLATES-FORTIFIED COMMERCIAL	DAY 7	+ ⊖	+ ⊖	<u>12/20/2006</u>
	DAY 14	+ ⊖	+ ⊖	<u>12/27/2006</u>
	DAY 21	+ ⊖	+ ⊖	<u>01/03/2007</u>
AGAR PLATES-MODIFIED HAYFLICK	DAY 7	+ ⊖	+ ⊖	<u>12/20/2006</u>
	DAY 14	+ ⊖	+ ⊖	<u>12/27/2006</u>
	DAY 21	+ ⊖	+ ⊖	<u>01/03/2007</u>
AGAR PLATES-HEART INFUSION	DAY 7	+ ⊖	+ ⊖	<u>12/20/2006</u>
	DAY 14	+ ⊖	+ ⊖	<u>12/27/2006</u>
	DAY 21	+ ⊖	+ ⊖	<u>01/03/2007</u>
BROTH SUBCULTURES (DAY 7)		DATE: <u>12/20/2006</u>		
AGAR PLATES-FORTIFIED COMMERCIAL	DAY 7	+ ⊖	+ ⊖	<u>12/27/2006</u>
	DAY 14	+ ⊖	+ ⊖	<u>01/03/2007</u>
	DAY 21	+ ⊖	+ ⊖	<u>01/10/2007</u>
AGAR PLATES-MODIFIED HAYFLICK	DAY 7	+ ⊖	+ ⊖	<u>12/27/2006</u>
	DAY 14	+ ⊖	+ ⊖	<u>01/03/2007</u>
	DAY 21	+ ⊖	+ ⊖	<u>01/10/2007</u>
AGAR PLATES-HEART INFUSION	DAY 7	+ ⊖	+ ⊖	<u>12/27/2006</u>
	DAY 14	+ ⊖	+ ⊖	<u>01/03/2007</u>
	DAY 21	+ ⊖	+ ⊖	<u>01/10/2007</u>

RESULTS: No detectable mycoplasmal contamination

1/10/07  
 Date



**M-250 Procedural Summary:** The objective of this test is to ascertain whether or not detectable mycoplasmas are present in an in vitro cell culture sample, be it a primary culture, hybridoma, master seed stock or cell line. This procedure combines an indirect DNA staining approach to detect non-cultivable mycoplasmas with a direct culture methodology utilizing three different mycoplasma media formulations. The indirect approach involves the inoculation of the sample into a mycoplasma-free VERO (ATCC) indicator cell line and performing a DNA fluorochrome assay after 72-120 hours of incubation. The direct culture aspect of the test utilizes three different mycoplasma media including both broth and agar formulations. The sample is inoculated into each of the 3 broth formulations and also onto duplicate plates (0.1 ml/plate) for each of the 3 agar formulations. Subculture from broth to fresh agar plates is carried out after 7 days incubation. Agar plates are incubated aerobically and microaerophilically in order to detect any colony forming units morphologically indicative of mycoplasma contamination. Issuance of the final report with signature of the Scientific Director/Study Director signifies that the required controls were performed concurrently with the test sample(s) as detailed in the referenced SOPs and that all test conditions have been found to meet the required acceptance criteria for a valid test, including the appropriate results for the positive and negative controls.

**Report Date:** December 15, 2006

**Case Details:**

**Cell Line:** H1 lot 10

**Passage #:** 24

**Date Completed:** 12/15/06

**Cell Line Gender:** Male

**Investigator:** [REDACTED]

**Specimen:** hES on MEF feeder

**Date of Sample:** 12/13/2006


**Tests, Reason for:** G-Banded chromosome analysis, Testing for karyotypic integrity of H1 Lot 10 p24 for Distribution

**Results:** 46,XY

**Completed by:** [REDACTED] CLSp(CG), on 15-Dec-06

**Reviewed and interpreted by:** [REDACTED] PhD, FACMG, on 15-Dec-06

**Interpretation:** No abnormalities were detected at the standard level of resolution.

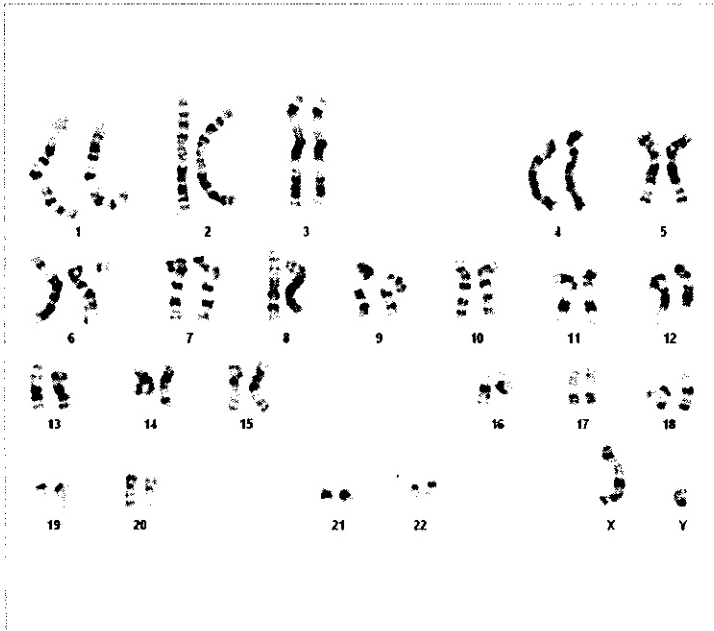

**Cell:** S01-04

**Slide:** A

**Slide Type:** Karyotyping

**Cell Results:** Karyotype: 46,XY

**# of Cells Counted:** 20

**# of Cells Karyotyped:** 7

**# of Cells Analyzed:** 9

**Band Level:** 400-500